


# When to “SNAP”<sup>®</sup>”

Snap the device just as the blue activation circle begins to disappear.

Be sure to snap the device down firmly so the top is completely flush with the base.

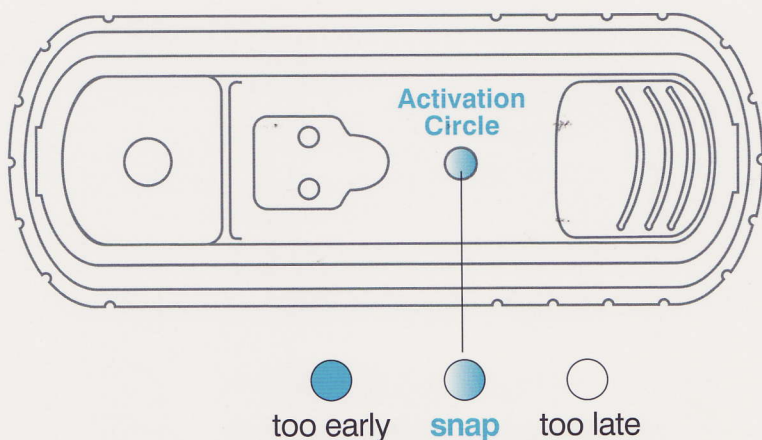

## After adding the sample to the sample well:

- Sample flow rate to the activation circle should take 30-60 seconds.
- A flow longer than 60 seconds may be the result of pipetting less than 450  $\mu$ l of the milk sample, or a very thick milk sample.
- A flow rate longer than 60 seconds may result in an inaccurate test result.

**IDEXX**