


When to “SNAP”[®]”

Snap the device just as the blue activation circle begins to disappear.

Be sure to snap the device down firmly so the top is completely flush with the base.

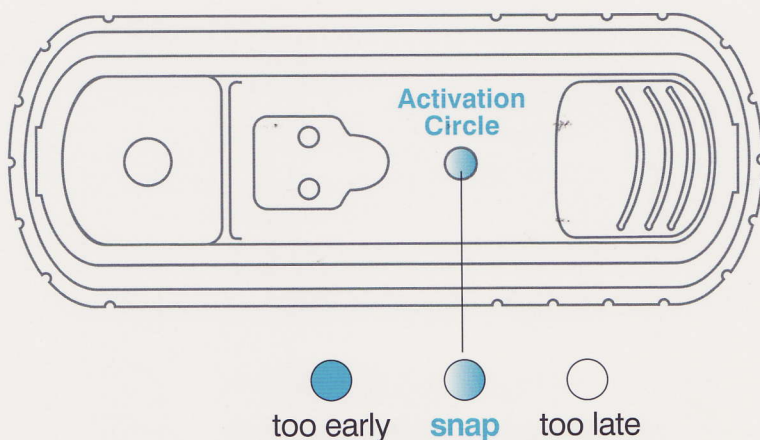

After adding the sample to the sample well:

- Sample flow rate to the activation circle should take 30-60 seconds.
- A flow longer than 60 seconds may be the result of pipetting less than 450 μ l of the milk sample, or a very thick milk sample.
- A flow rate longer than 60 seconds may result in an inaccurate test result.

IDEXX